


Certificate of Factory Calibration

1/4" IEPE Free Field Measurement Microphone
Type : MI17
Serial No. : 146
Sensitivity : 50.6 mV/Pa (@ 1 kHz | 22°C | 1015 hPa)

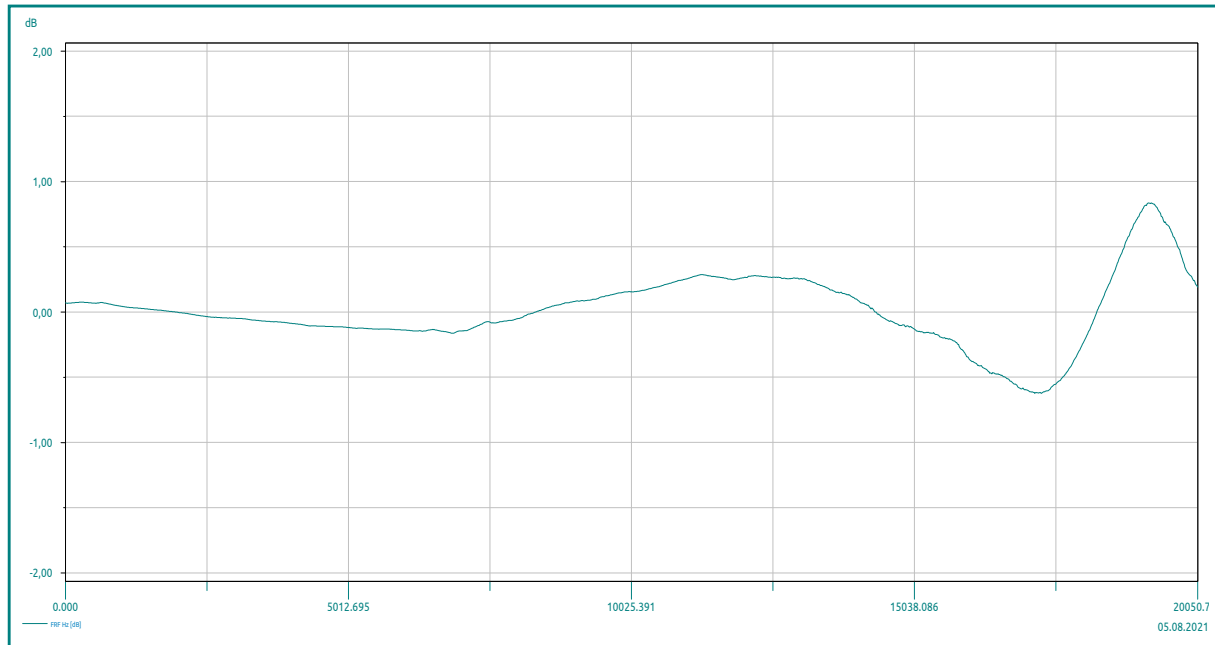

BSWA Full Frequency Coupler CA916 # 540002
Reference Microphone # MPA231
Svantek SV30A # 14126
Plug.n.DAQ Lite # 353
Software : DASyLab Pro 2020.1

Calibrated by

Rogá

