


Certificate of Factory Calibration

1/4" IEPE Free Field Measurement Microphone
Type : AVM MI17SW
Serial No. : 1417
Sensitivity : 52.7 mV/Pa (@ 1 kHz | 20 °C | 1022 hPa)

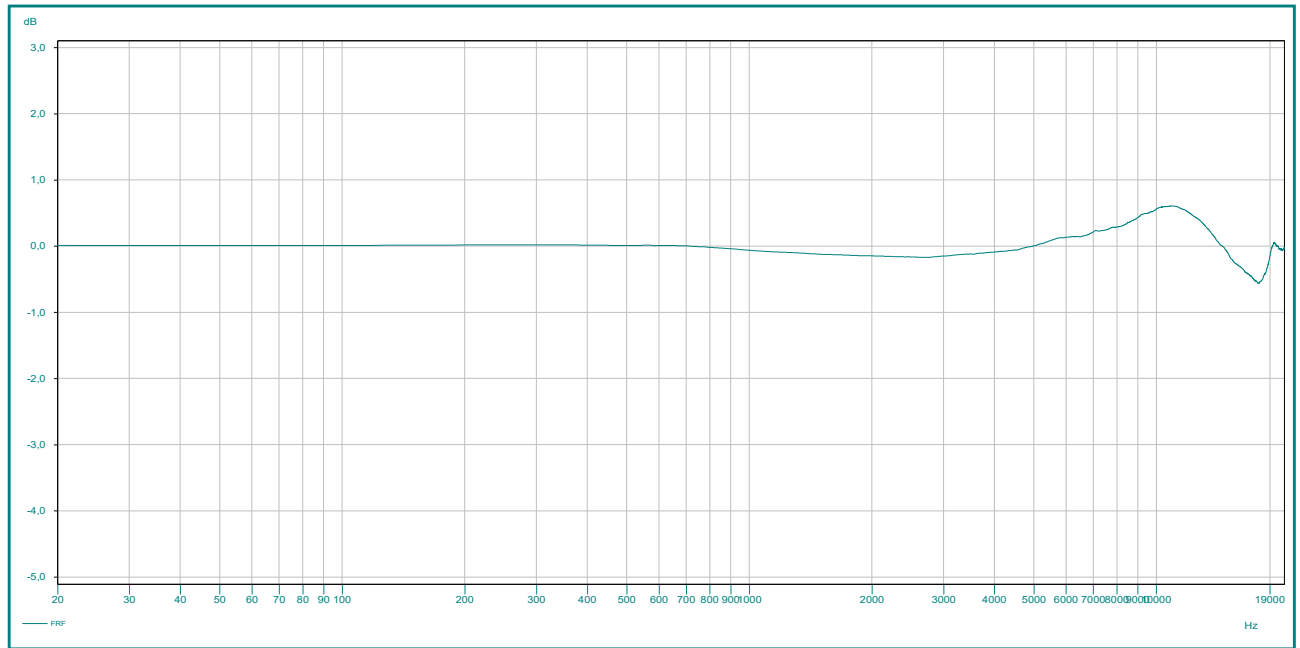

BSWA Full Frequency Coupler CA916	540002
Reference Microphone	MPA231
Svantek SV30A	14126
Plug.n.DAQ Lite	353
Software : DASyLab Pro	2020.1
Measurement uncertainty	0.20 dB

Calibrated by

Roga, 15.01.2022

